

# How to use an iPad to share data with your clinic

Do you want to use the Dexcom receiver as your primary display device but want to use the Dexcom G7 app on your iPad to send data to your clinic? If so, these instructions are for you.

## STEP 1: SETUP DEXCOM RECEIVER

- 1 Press and hold the **Select** button for 3–5 seconds to turn receiver on.
- 2 Go through the receiver setup. The receiver walks you through setup step-by-step.



## STEP 2: CREATE DEXCOM ACCOUNT AND SETUP DEXCOM G7 APP

- 1 Download the Dexcom G7 app on your iPad. If you have a VA supplied iPad go to the Hub to find the Dexcom G7 app.
- 2 Create a Dexcom Account. Use your email or phone number to sign up for an account.
- 3 Go through the app setup screens to automatically connect to your sensor session in progress. You will need the sensor code of the sensor you are wearing.





### TIPS

- Don't close the Dexcom G7 app on your iPad.
- Open the Dexcom G7 app on your iPad every 24 hours and make sure your sensor is connected to it. This will make sure all your data is being sent to Dexcom Clarity.
- Connect your sensor to both your receiver and the Dexcom G7 app on the iPad every time you start a new sensor.
- Keep your iPad charged and do not turn it off.
- Turn off Signal Loss notification under **Profile > Alerts > Signal Loss** to avoid getting unwanted notifications.

## STEP 3: SHARE DATA WITH YOUR CLINIC

You can authorize data sharing with your clinic so they have access to your data. Your clinic will provide you with a clinic code. To begin sharing data:

- 1 In the Dexcom G7 app tap **Connections > Clarity Clinic**.
- 2 Follow the instructions to enter the clinic code.

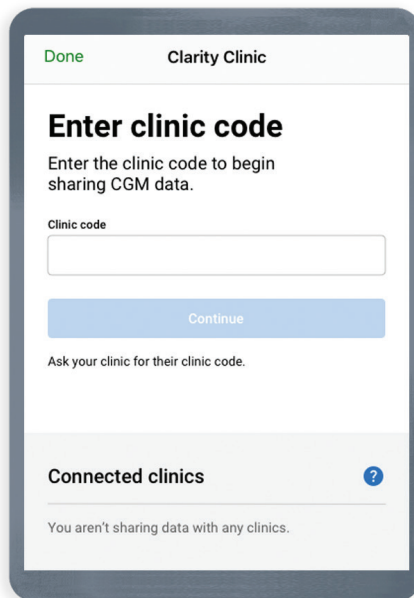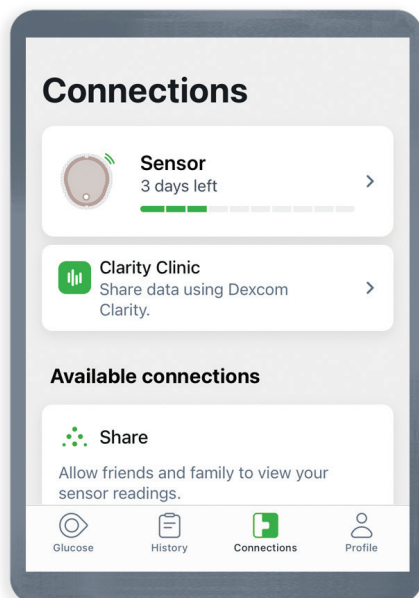

**BRIEF SAFETY STATEMENT:** Failure to use the Dexcom Continuous Glucose Monitoring System and its components according to the instructions for use provided with your device and available at <https://www.dexcom.com/safety-information> and to properly consider all indications, contraindications, warnings, precautions, and cautions in those instructions for use may result in you missing a severe hypoglycemia (low blood glucose) or hyperglycemia (high blood glucose) occurrence and/or making a treatment decision that may result in injury. If your glucose alerts and readings from the Dexcom CGM do not match symptoms, use a blood glucose meter to make diabetes treatment decisions. Seek medical advice and attention when appropriate, including for any medical emergency.

**BRIEF SAFETY STATEMENT:** The web-based Dexcom Clarity software is intended for use by both home users and healthcare professionals to assist people with diabetes and their healthcare professionals in the review, analysis, and evaluation of historical CGM data to support effective diabetes management. It is intended for use as an accessory to Dexcom CGM devices with data interface capabilities. Caution: The software does not provide any medical advice and should not be used for that purpose. Home users must consult a healthcare professional before making any medical interpretation and therapy adjustments from the information in the software. Caution: Healthcare professionals should use information in the software in conjunction with other clinical information available to them. Caution: Federal (US) law restricts this device to sale by or on the order of a licensed healthcare professional.

Dexcom, Dexcom Clarity, Dexcom Follow, Dexcom One, Dexcom Share, Stelo, and any related logos and design marks are either registered trademarks or trademarks of Dexcom, Inc. in the United States and/or other countries.

©2025 Dexcom, Inc. All rights reserved. MAT-0325 v4.0